



## → MEASUREMENTS AND OBSERVATIONS IN THE 21<sup>st</sup> CENTURY CONFERENCE

# Open hardware portable dual-probe heat-pulse sensor for measuring soil thermal properties and water content

Giovanni Ravazzani



**POLITECNICO**  
MILANO 1863

DIPARTIMENTO DI  
INGEGNERIA CIVILE E AMBIENTALE

21 November 2016 | ESA-ESRIN | Frascati (Rome) Italy

## MOTIVATION

- Assessment of thermal soil properties, useful in many hydrological fields such as estimate of river-groundwater interaction or soil moisture estimation from satellite images using the thermal inertia method.
- Available portable equipments are very expensive, despite the basic methods to measure thermal properties are easy to implement. Measuring technique requires lots of energy, so batteries are short-lasting





## OBJECTIVE

- To build a low cost, portable, long-lasting device based on open-hardware technologies, for measuring soil thermal properties.



# Theoretical background

Heat pulse of finite duration, emitted from a heat source.  
Temperature rise recorded at a known distance from the emitter.



$$\Delta T(r, t) = \begin{cases} -\frac{Q'}{4\pi\kappa} Ei\left(\frac{-r^2}{4\kappa t}\right) & 0 < t \leq t_0 \\ \frac{Q'}{4\pi\kappa} \left\{ Ei\left[\frac{-r^2}{4\kappa(t-t_0)}\right] - Ei\left(\frac{-r^2}{4\kappa t}\right) \right\} & t > t_0 \end{cases}$$

where  $t$  is time from beginning of heating,  $Q'$  is the source strength per unit time ( $\text{m}^2 \text{K s}^{-1}$ ),  $\kappa$  is the thermal diffusivity ( $\text{m}^2 \text{s}^{-1}$ ) of the medium surrounding the heater, and  $-Ei(-x)$  is the exponential integral function with argument  $x$ .  $Q'$  is defined as  $Q' = q'/\rho c$ , where  $q'$  is the energy input per unit length of heater per unit time ( $\text{W m}^{-1}$ ) and  $\rho c$  is the volumetric heat capacity ( $\text{J m}^{-3} \text{K}^{-1}$ ).

# The single point method

Volumetric heat capacity ( $\text{J m}^{-3} \text{K}^{-1}$ )


$$\rho c = \frac{q'}{4\pi\kappa\Delta T_m} \left\{ Ei \left[ \frac{-r_n^2}{4\kappa(t_m - t_0)} \right] - Ei \left( \frac{-r_n^2}{4\kappa t_m} \right) \right\}$$

Thermal diffusivity ( $\text{m}^2 \text{s}^{-1}$ )

$$\kappa = \frac{r_n^2}{4} \left\{ \frac{1/(t_m - t_0) - 1/t_m}{\ln[t_m/(t_m - t_0)]} \right\}$$


Thermal conductivity ( $\text{W m}^{-1} \text{K}^{-1}$ )

$$\lambda = \kappa \cdot \rho c$$



where  $r_n$  is the needle spacing of the DPHP (m),  $t_m$  is the time of the maximum temperature change (s), and  $\Delta T_m$  is the maximum temperature increase (K) as recorded from the DPHP thermistor.

# Soil moisture



Source: Canot É, et al. ASME. J.  
Heat Transfer. 2016

Fraction of soil solid

Heat capacity of water

$$\rho c = (\rho c)_s \phi_s + (\rho c)_w \mathcal{G}_v$$

Heat capacity of soil solid

**Unknown: water content**


Volumetric heat capacity of soil can be determined as the sum of the heat capacity of water and solid, ignoring contribution given by air and defining solid to include the mineral and organic matter fractions, where  $\phi_s$  is the volume fraction of soil (= (1-P) with soil porosity),  $(\rho c)_s$  is the volumetric heat of soil solid,  $(\rho c)_w$  is the volumetric heat of water, and  $\mathcal{G}_v$  is the volumetric water content. Because  $(\rho c)_w$  is known, measurement of  $\rho c$  obtained with the multi-needle probe can be used together with estimates or measurements of volumetric heat of soil to obtain  $\mathcal{G}_v$ .



# The developed equipment



# Correction for transient ambient temperature





# Sensor spacing calibration



agar-stabilized water (5 g L<sup>-1</sup>) (21° C)

$$\lambda = 0.60106 \text{ Wm}^{-1}\text{K}^{-1}$$

$$\rho c = 4174000 \text{ Jm}^{-3}\text{s}^{-1}$$

Apparent probe spacing is calibrated against measurement on medium with known thermal properties, such as water.


$\Delta T_m$	$t_m$	$q'$	$r$	$\rho c$	$\lambda$	$\varepsilon_{\rho c}$	$\varepsilon_{\lambda}$
0.595	63.1	82.8	0.005705	4003	0.55272	4.10	8.04
0.601	62.28	81.87	0.005654	3988	0.54871	4.45	8.71
0.604	63.28	81.87	0.005672	3944	0.53673	5.50	10.70
0.572	63.08	81.64	0.005741	4054	0.56709	2.87	5.65
0.573	64.58	81.42	0.005770	3995	0.55053	4.30	8.41
0.598	63.98	81.19	0.005691	3924	0.53131	5.98	11.60
0.585	63.48	80.5	0.005698	3967	0.54305	4.95	9.65




# Laboratory test: soil moisture estimate

## Experimental setup

Volume and dimensions of the two types of containers were chosen in such a way that they are compatible to probe size and that measurements are representative of the entire soil sample



# Laboratory test: soil moisture estimate

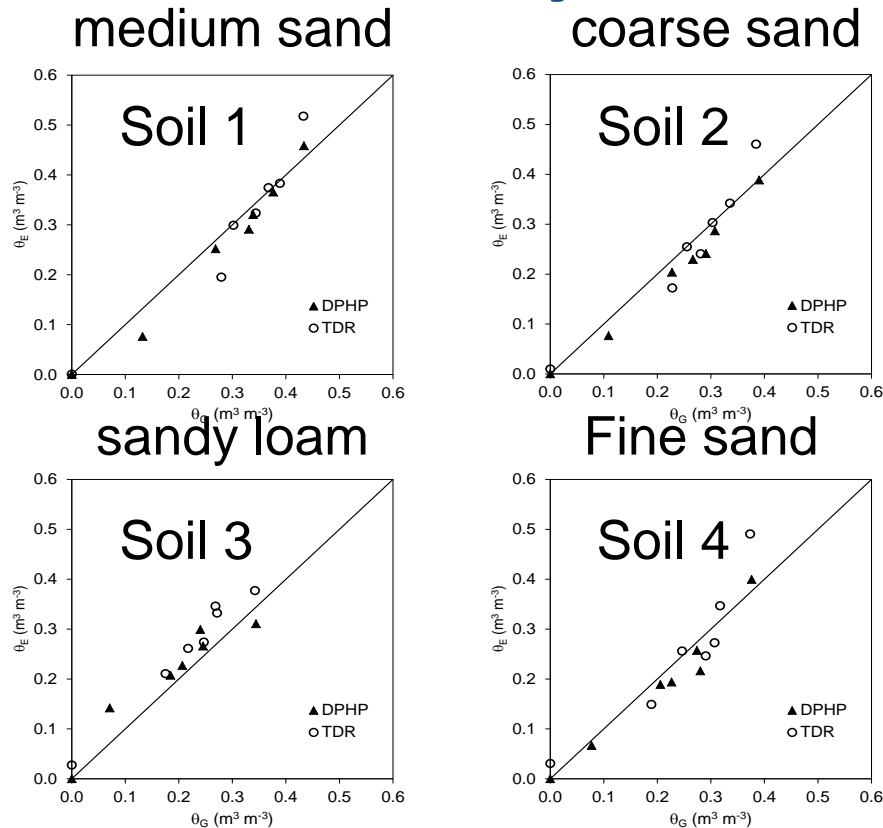

Soil ID	Heat capacity ( $\text{MJ m}^{-3} \text{K}^{-1}$ )	CV
1	$2.392 \pm 0.093$	3.9
2	$2.459 \pm 0.085$	3.5
3	$2.494 \pm 0.065$	2.6
4	$2.723 \pm 0.044$	1.6

Soil ID	DPHP			TDR		
	MPE	MAPE	NMSE	MPE	MAPE	NMSE
1	-0.0953	0.1141	0.014	-0.0267	0.0984	0.027
2	-0.1134	0.1134	0.019	-0.0286	0.1008	0.027
3	0.2212	0.2536	0.045	0.1543	0.1543	0.040
4	-0.0849	0.1056	0.026	-0.0113	0.1469	0.054



## Conclusions

- The open hardware platform is good for self-building low cost device for soil thermal properties assessment.
- The DPHP probe showed an accuracy comparable to TDR in estimating water content, but the DPHP can be used to investigate smaller volume of soil.
- The counterpart is that TDR is much faster than DPHP in measure acquisition.

# Future developments

- Develop a new version based on a more powerful board
- Implement different methods to estimate thermal parameters from temperature rise
- Include a GPS unit to log position of measurements during a field campaign





Thank you for your  
attention

*This presentation available on  
[www.ravazzani.it](http://www.ravazzani.it)*

# Laboratory test: soil moisture estimate

Description, origin, median grain size,  $D_{50}$  (mm), coefficient of uniformity, CU, computed as the ratio between the grain diameter at 60% passing, and the grain diameter at 10% passing, porosity ( $\text{m}^3/\text{m}^3$ ), and bulk density ( $\text{Mg m}^{-3}$ )

Soil ID	Description	Origin	$D_{50}$ (mm)	CU	Porosity ( $\text{m}^3/\text{m}^3$ )	Bulk density ( $\text{Mg m}^{-3}$ )
1	Medium sand	River Toce, Vogogna-Prata	0.30	3.25	0.434	1380
2	Coarse sand	River Toce, Masone	0.45	4.83	0.390	1460
3	Sandy loam	Cultivated field, Bibione	0.20	5.00	0.344	1464
4	Fine sand	Beach, Bibione	0.22	3.79	0.376	1606